


PROMARK ☆☆☆☆☆ IMAGING

UltraMaxx MDP

*The Industry's Best
Direct Radiographic Detector
For Radiographic Medical Imaging*


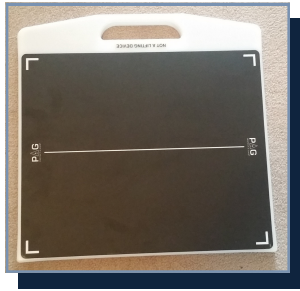


CsI Cesium Iodide

Cassette Sized!
UltraHigh Resolution!
Auto Exposure Detection!

Highly Acclaimed METRON Acquisition and Review Software with exclusive Guided and Free Mark Up Routines and comprehensive on line support including Narrated Online Video Training Clips! Full Dicom 3.0 MWL and Send features standard!

On Line Support AND Narrated Training Videos!

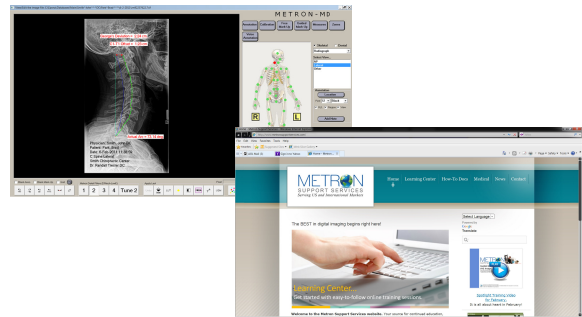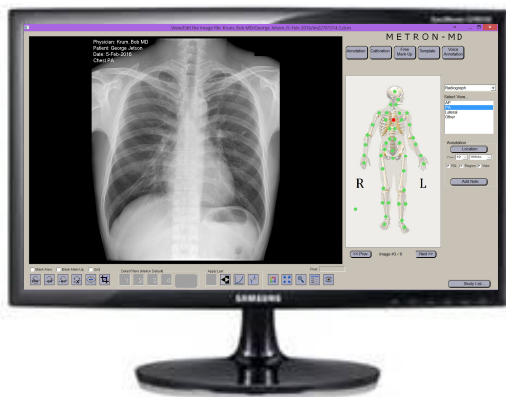

ULTRAMAXX-P Detector Specifications:

- *Image Matrix: 43x36 or 43x43cm ! 15/18 MEGA PIXELS!
- *CASSETTE SIZED PANEL! ISO4090 Standard
- *Sensor Type: a-Si TFT (Thin Film Transistors-Diode)
- *Direct Deposit Cesium Iodide (CSI-TI) *STANDARD*
- *AED - FULLY AUTOMATIC EXPOSURE DETECTION !
- *No connection to X-Ray Generator required
- *PIXEL PITCH 100 MICRON!
- *Resolution: Nominal 6.0 + lp/mm
- *Operating Temperature Range: 10 – 35 Degrees Celsius
- *WIRELESS OPTION !


Flexible DataBase Structure

Patient	Study Date	DOB	Physician	Im.	Sex	Status	Study ID
Khalid M (M)	30-Jan-2010	2-Jul-1985	Krum, Bob MD	2	M	Sent	2010130110261.1.1
Brian Bob	21-Jan-2010	5-Aug-1981	Krum, Bob MD	2	M	Sent	10121181101.1.1
Fred Flintstone	17-Jan-2010	1-Jan-2001	Krum, Bob MD	2	M	Sent	010111711044.1.1
Fred Flintstone	16-Jan-2010	1-Jan-2000	Krum, Bob MD	1	M	Sent	20101161102435.1.1
John Flintstone	21-Jan-2010	1-Jan-2000	Krum, Bob MD	9	M	Sent	2010121101600.1.1
Wilma Flintstone	16-Jan-2010	1-Jan-2000	Krum, Bob MD	1	M	Sent	20101161102092.1.1
Paul Costanzo	16-Jan-2010	1-Jan-2000	Krum, Bob MD	2	M	Sent	20101161102091.1.1
James T Kirk	16-Jan-2010	1-Jan-2000	Krum, Bob MD	1	M	Sent	20101161102082.1.1
James T Kirk	17-Jan-2010	1-Jan-2000	Krum, Bob MD	2	M	Sent	20101161102081.1.1
Barbara Nelson	13-Jul-2012	5-Sep-1971	Krum, Bob MD	2	F	Sent	2012171317272.1.1
James T Kirk	17-Jan-2010	1-Jan-2000	Krum, Bob MD	2	M	Sent	20101161102081.1.1
Luke Skywalker	5-Apr-2010	1-Jan-2000	Krum, Bob MD	2	M	Sent	20101211170.1.1
Arnold Zehi PhD	16-Jan-2010	1-Jan-2000	Krum, Bob MD	2	M	Sent	2010116110221.1.1
Arnold Zehi PhD	16-Jan-2010	1-Jan-2000	Krum, Bob MD	9	M	Sent	2010116110221.1.1

Metron MD Acquisition/Review Software:


- *Standard, Zoom, Pan, Scroll, Real Size View, Multi-View, Collections, Window/Level, Annotations etc.
- *Exposure Index and Technique Advisor
- *Advanced and Exclusive Guided and Free Mark Up routines
- *Advanced Image and Video Morphing
- *User Programmable Exposure Sequences
- *Two Additional View Station Licenses Included at no cost
- *DICOM PACS “Push/Pull” Q/R and Send Receive functions
- *CD/DVD Burning
- *Exclusive Send to WebViewer
- *Effortless Multiple Image Stitching
- *Auto-Scaler Tool for automatic computed measurement

Single or Multi View Review Window

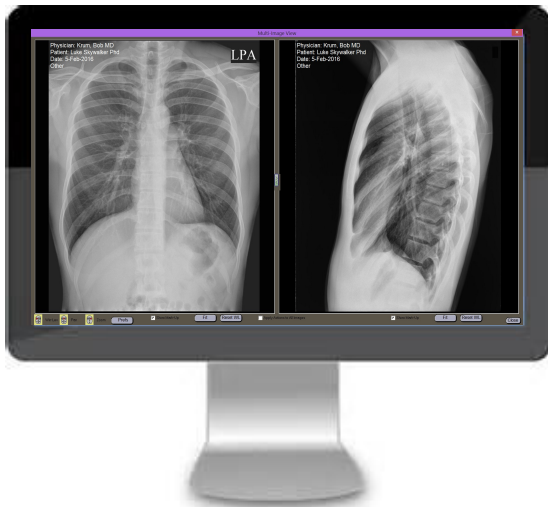


Appearance and specifications subject to change without notice


Flexible Report Generation

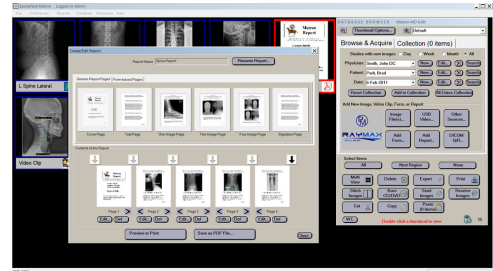


Comprehensive Free Mark Up

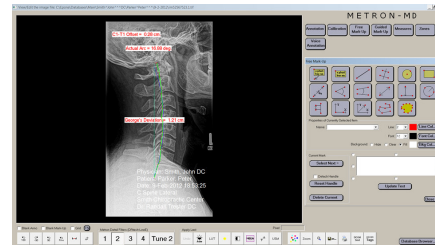

Easy CD/DVD Creation with mini Metron Viewer

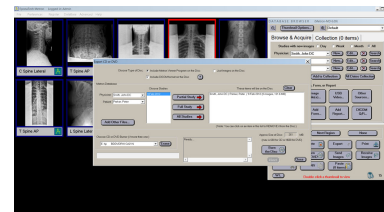

Patented Computed Guided Mark Up and zoning Routines

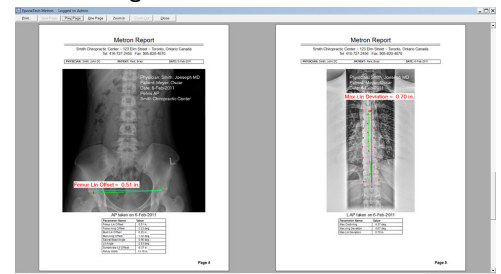

Promark Imaging
 1120 Finch Avenue West
 Suite 701-344
 Toronto, Ontario
 M3J 3H7, Canada
Ph. +1 416-727-2456
Fx. +1 905-820-4760
www.promarkimaging.com
info@promarkimaging.com